


2 / 32


FIG. 2

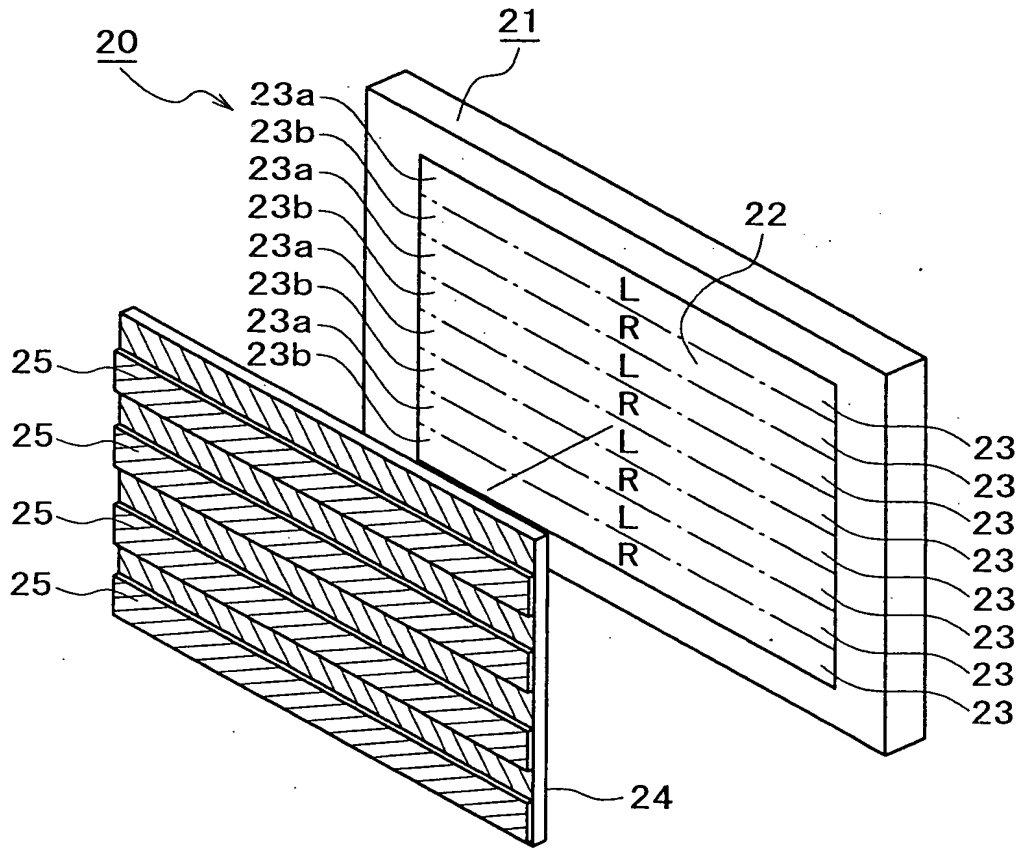

[illegible]


4 / 32

FIG. 4

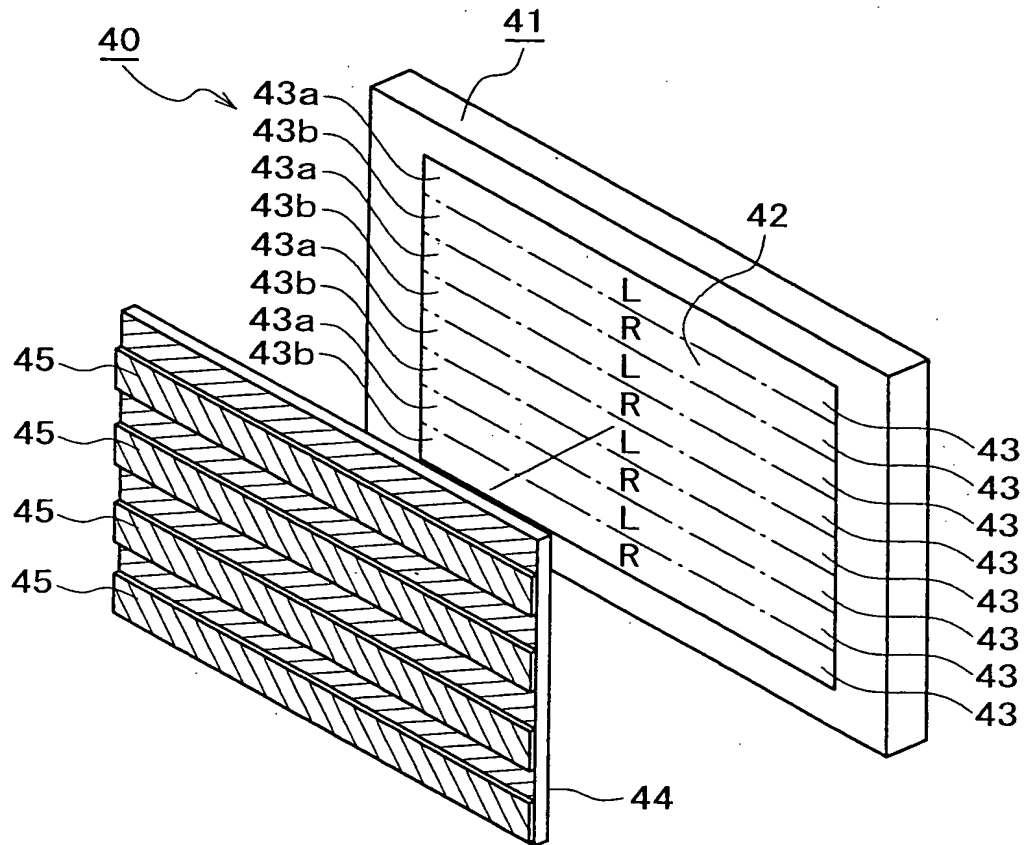


5/32

FIG. 5

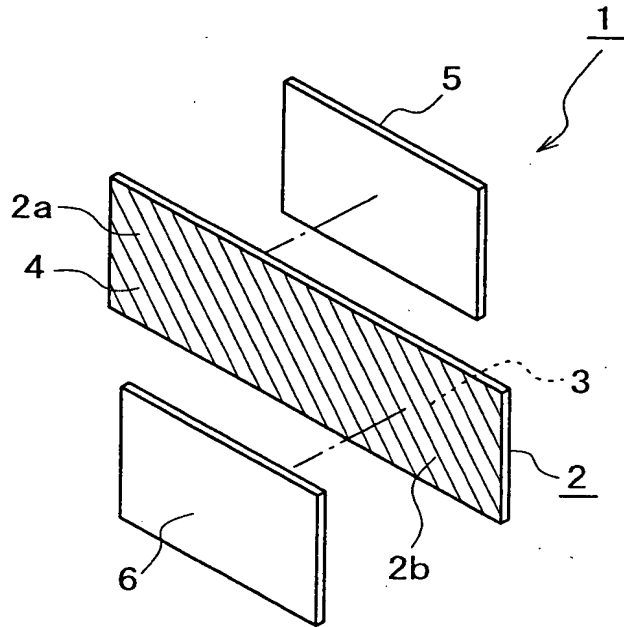


6/32

FIG. 6

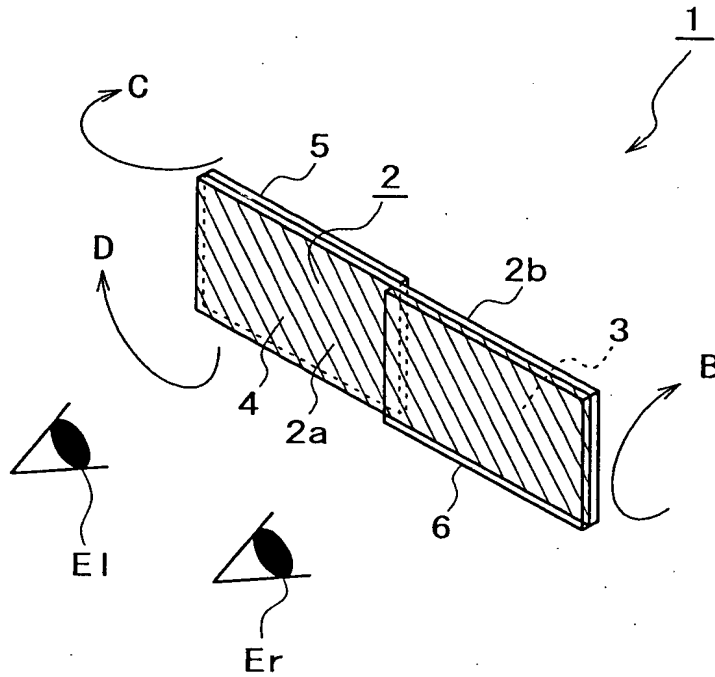


7/32

FIG. 7

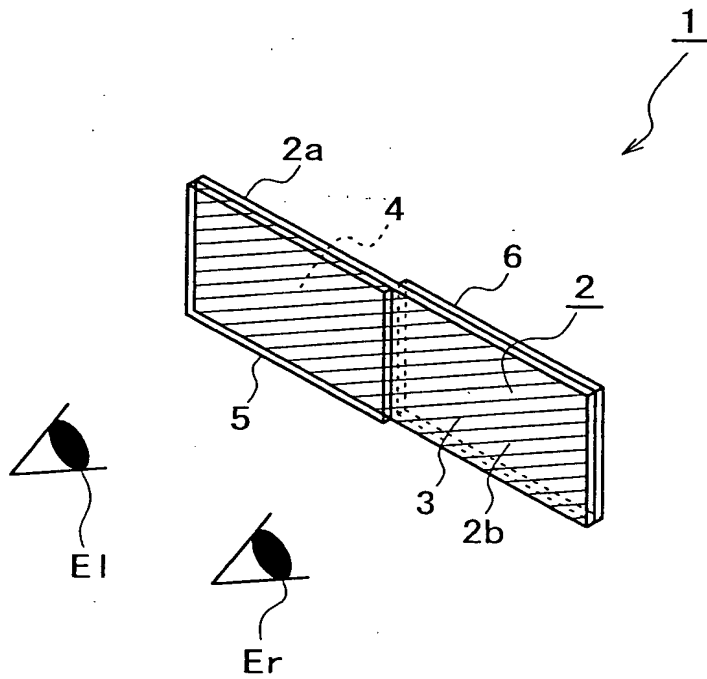


8/32

FIG. 8

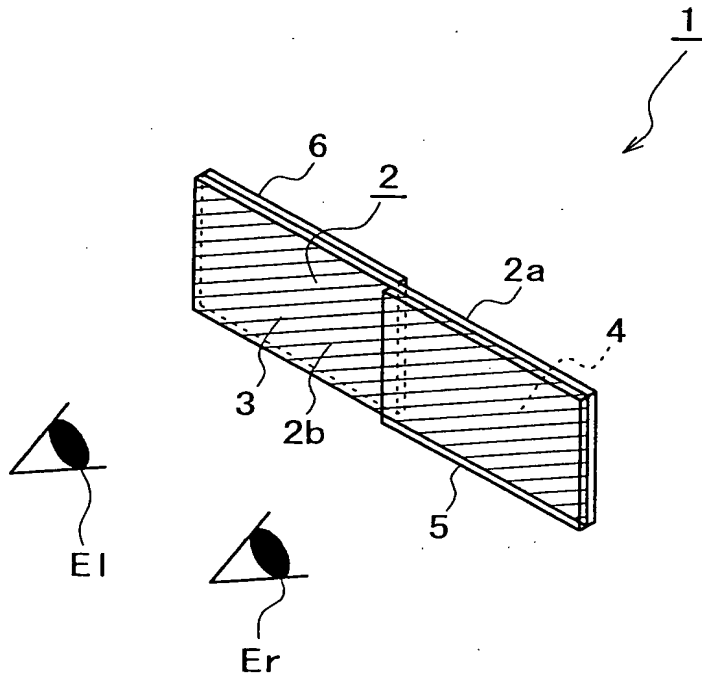


9/32

FIG. 9

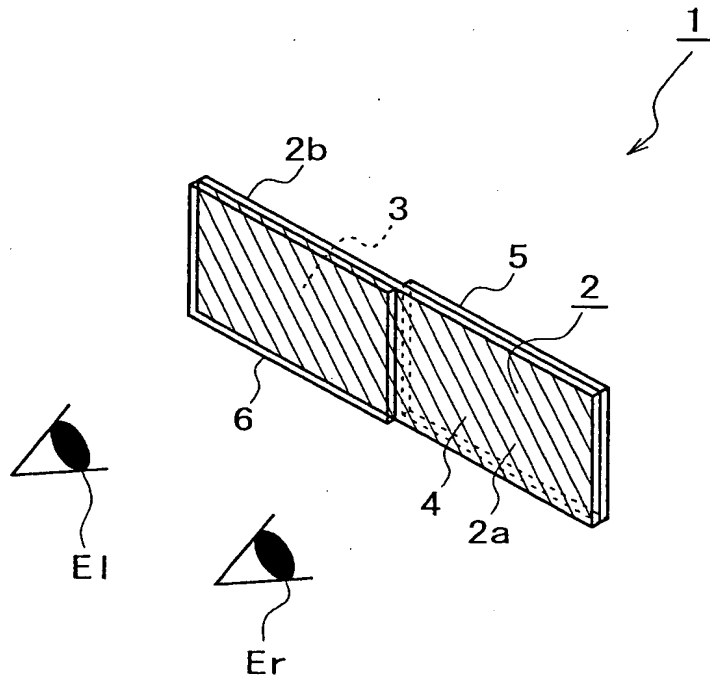

10/32

FIG. 10

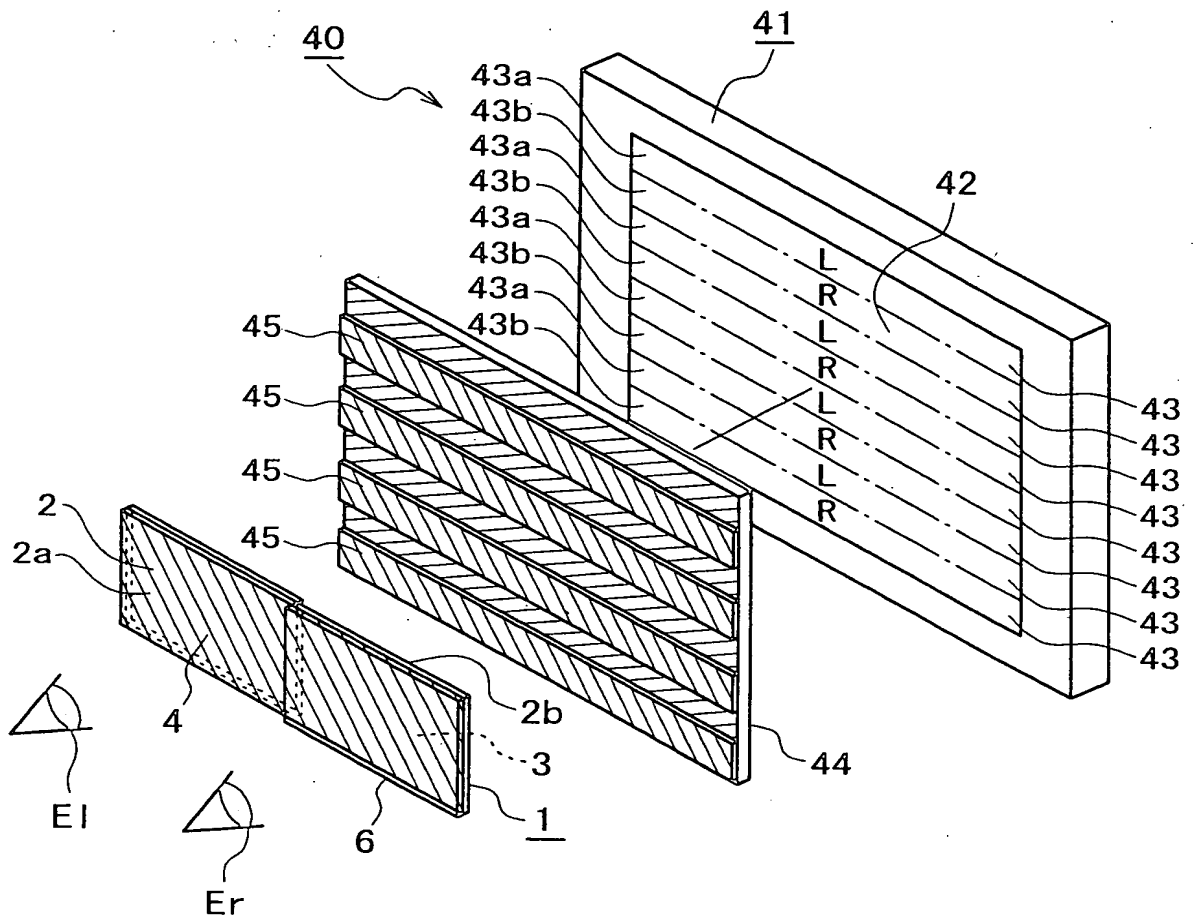

























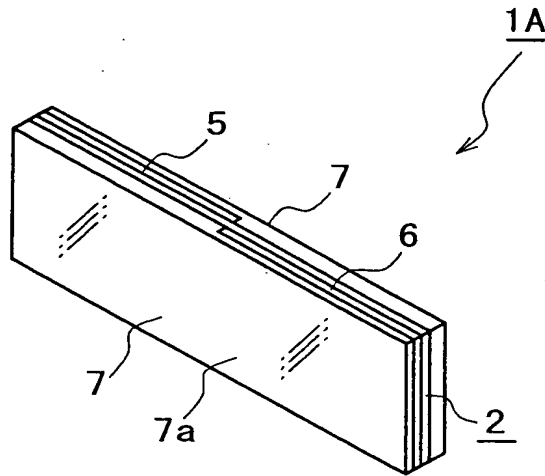
STEREOSCOPIC IMAGE DISPLAY APPARATUS					POLARIZING EYEGLASS DEVICE			
TYPE I	TYPE II	TYPE III	TYPE IV		SERVICE CONDITION A	SERVICE CONDITION B	SERVICE CONDITION C	SERVICE CONDITION D
								
								
								
								
								

FIG. 11


12/32

FIG. 12



13 / 32

FIG. 13

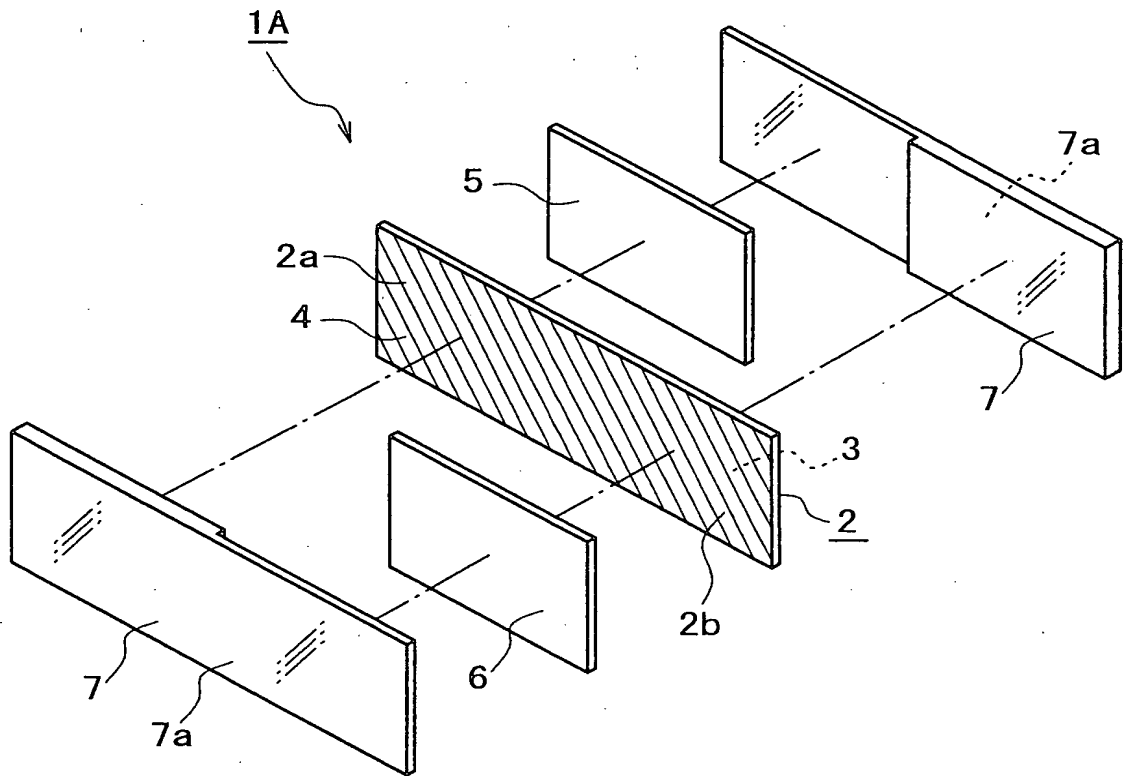

14 / 32

FIG. 14



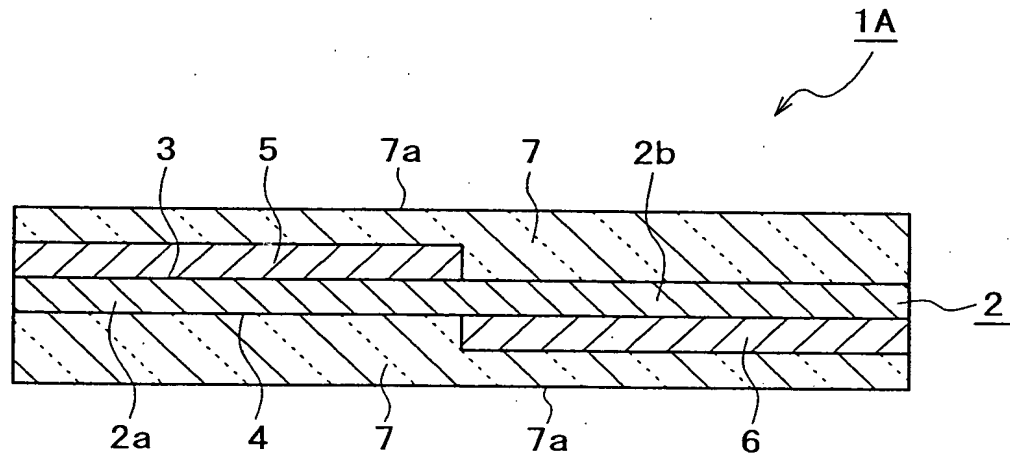


FIG. 15

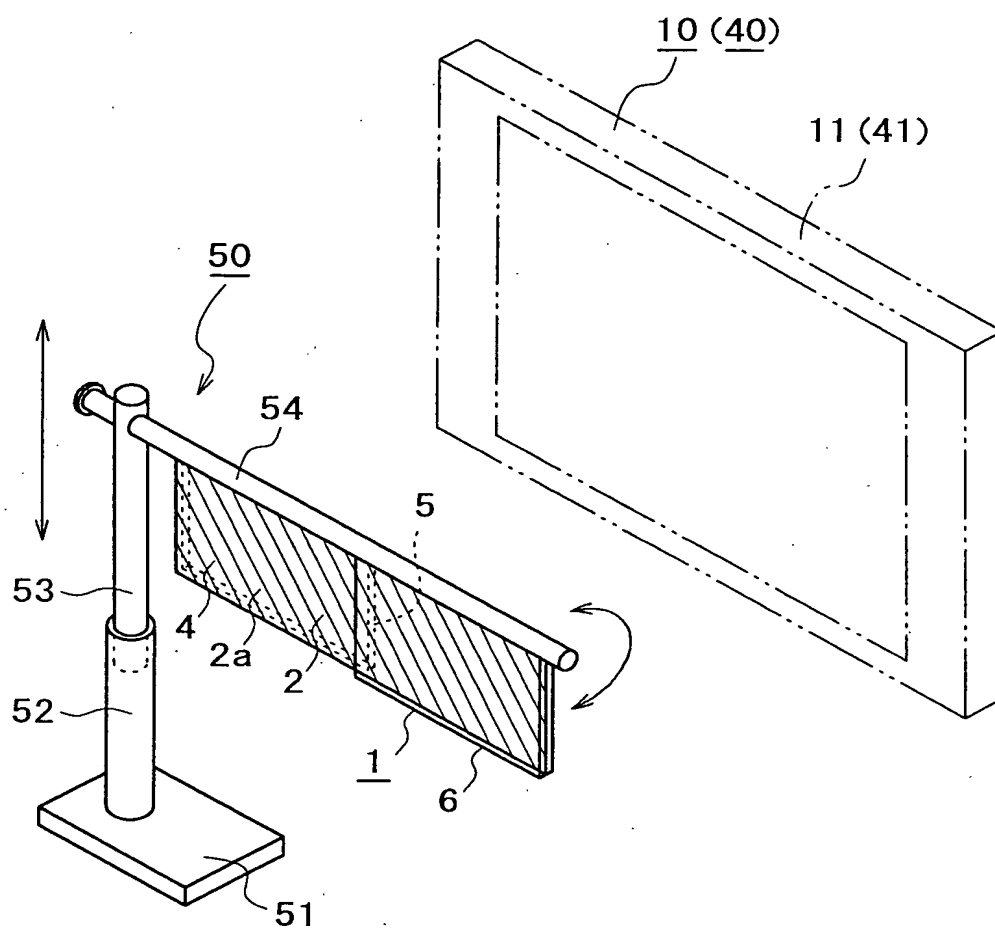


16/32

FIG. 16

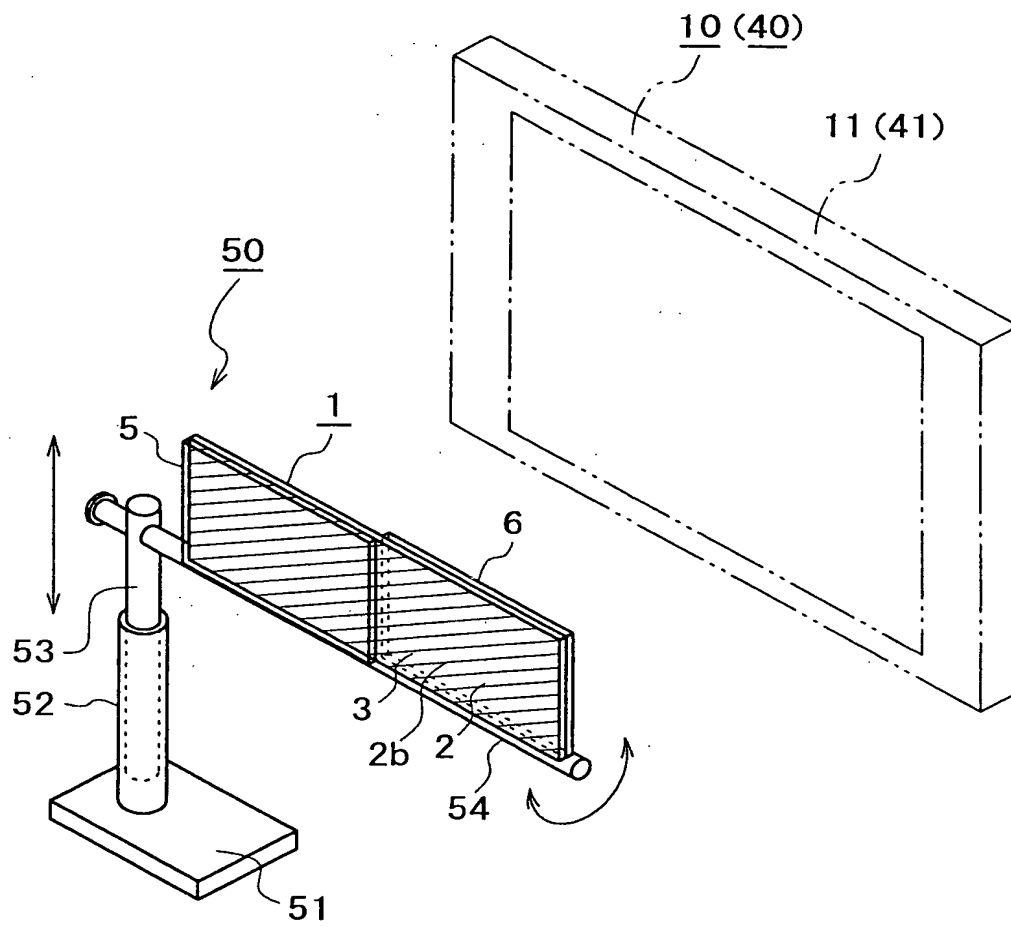

17/32

FIG. 17

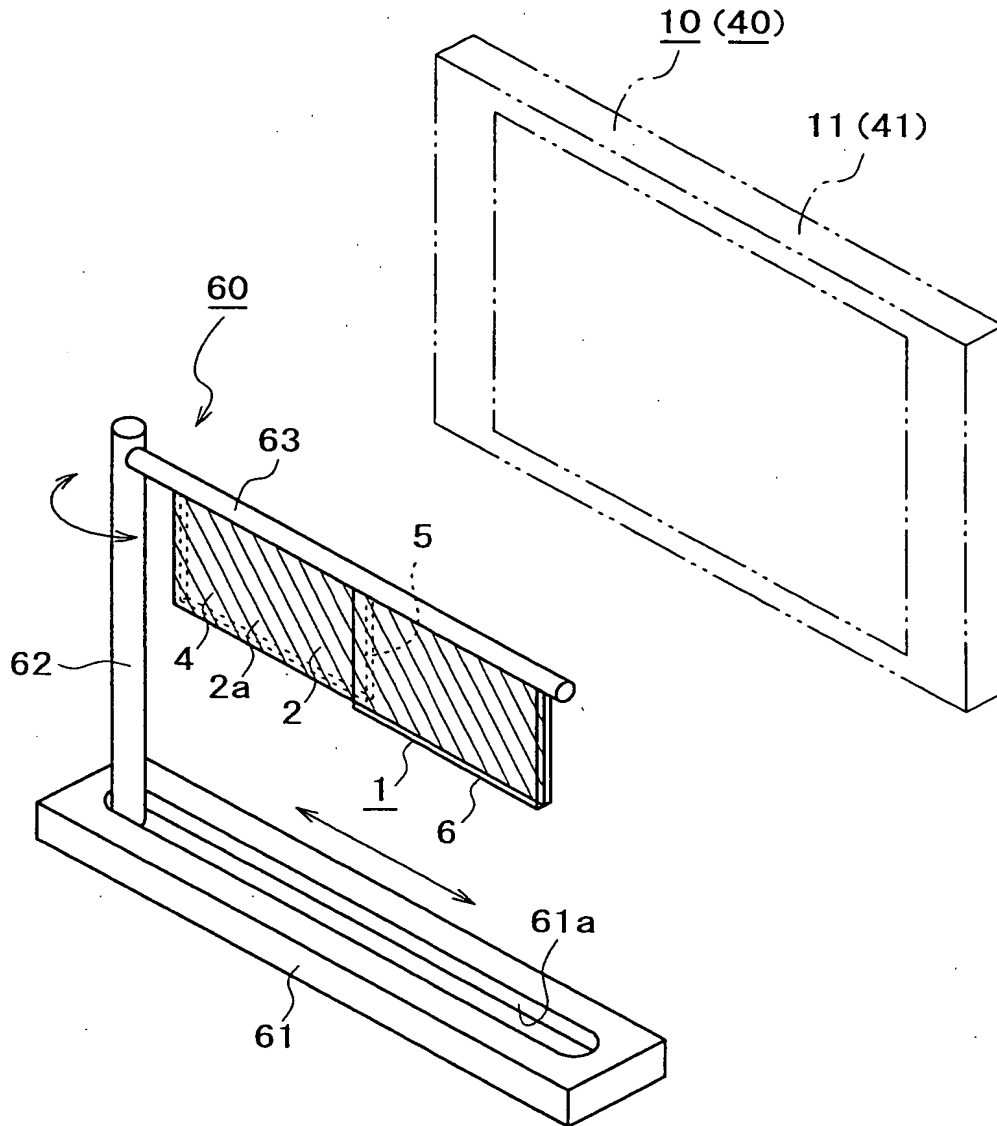

18/32

FIG. 18



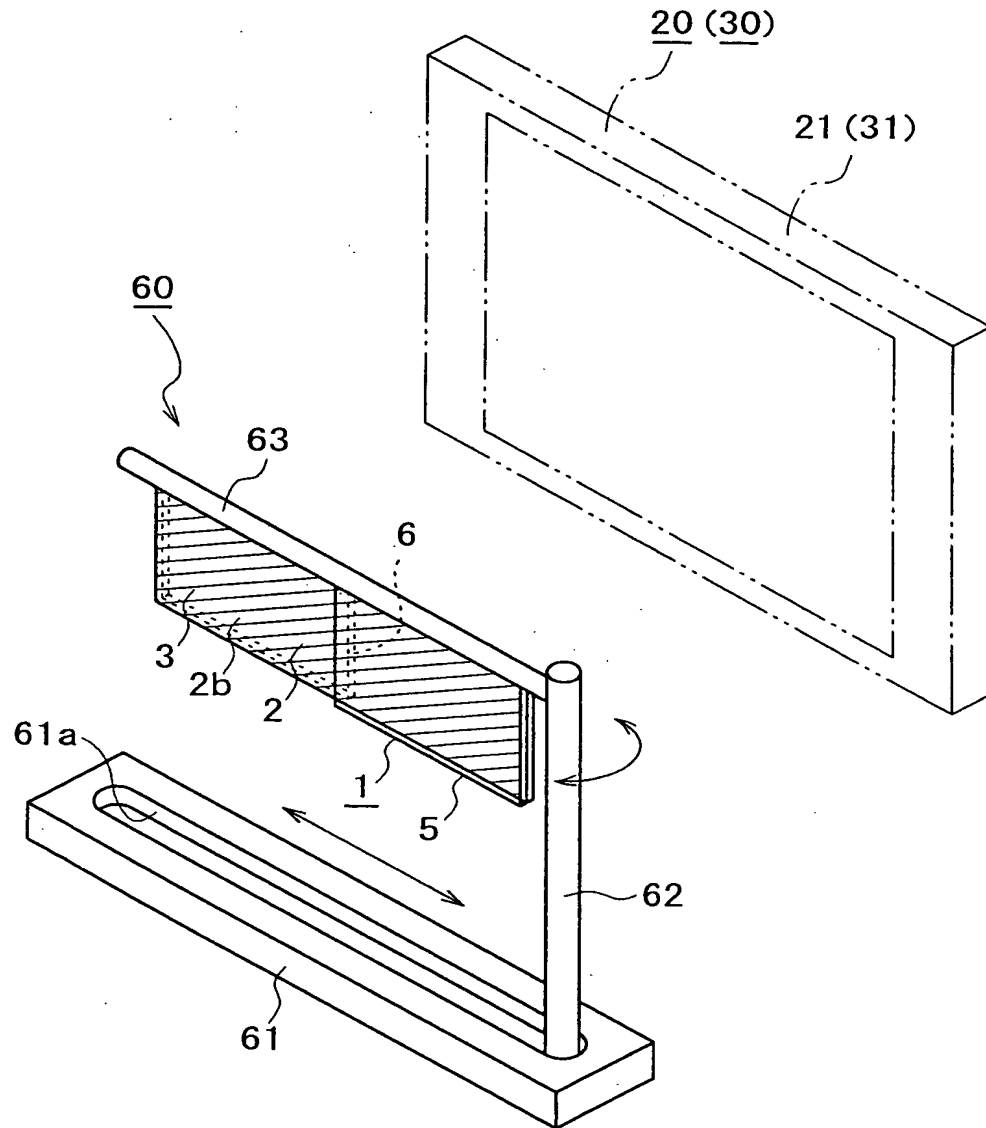


FIG. 19

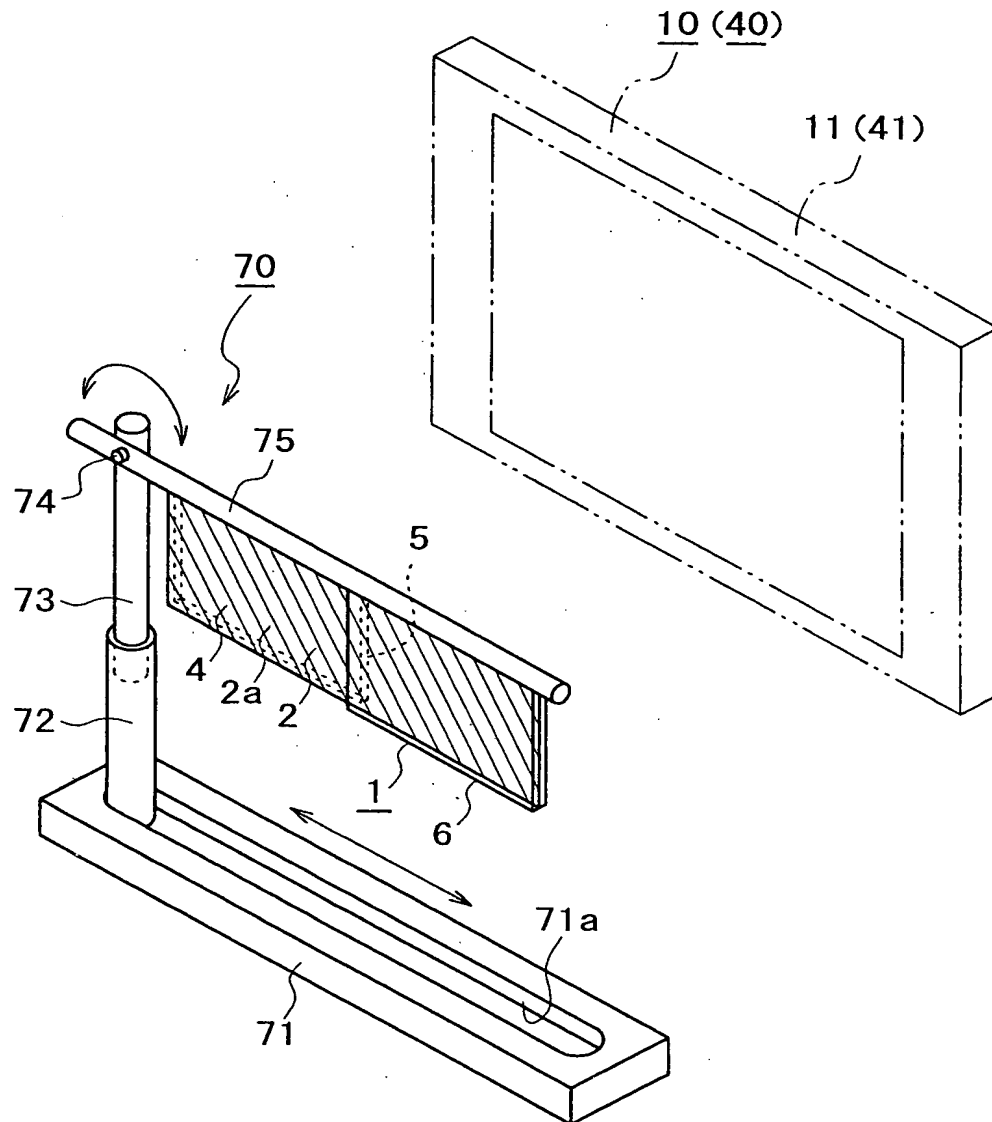

20/32

FIG. 20

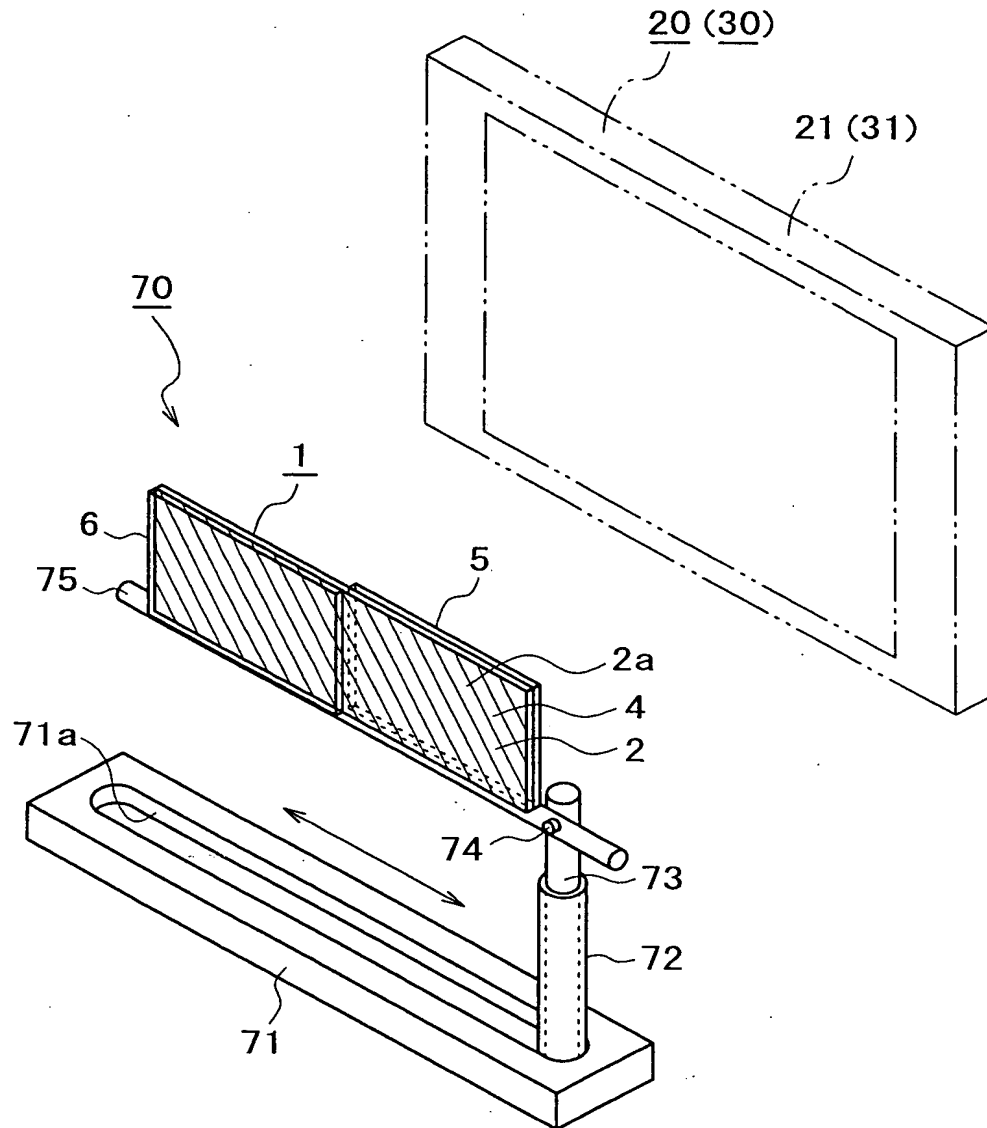

21/32

FIG. 21



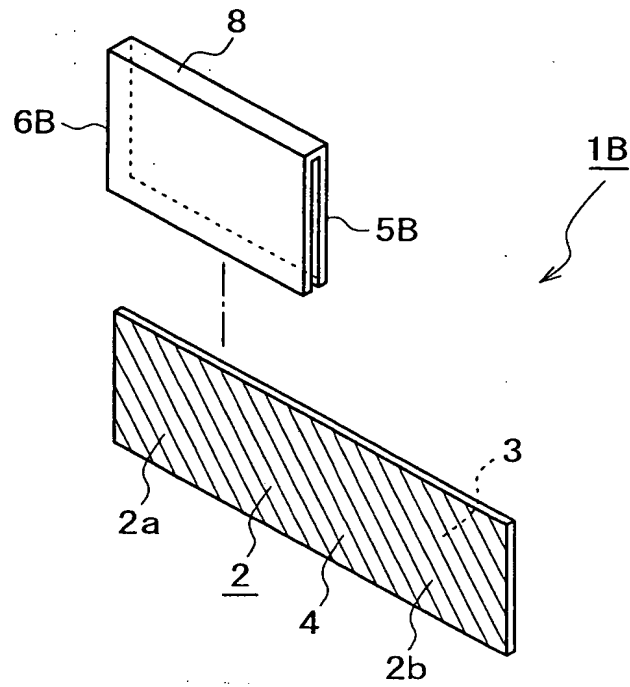


FIG. 22

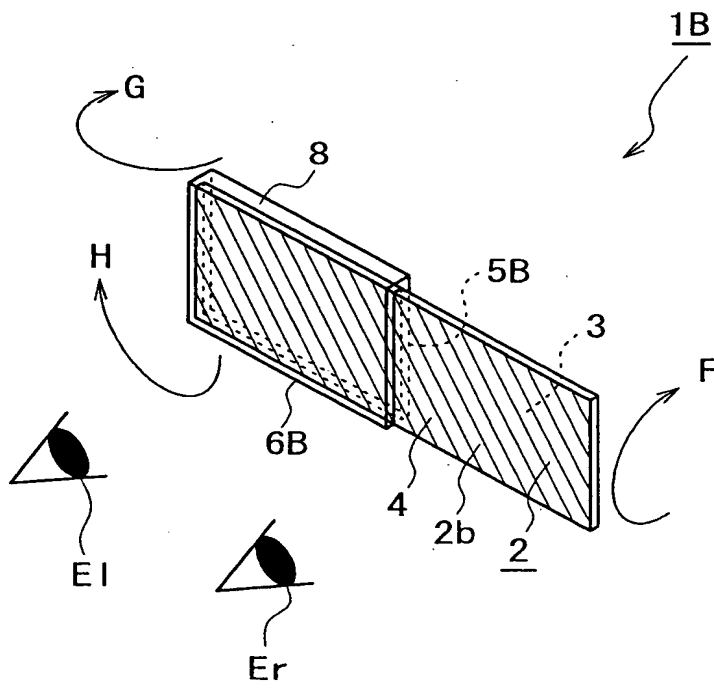


23 / 32

FIG. 23

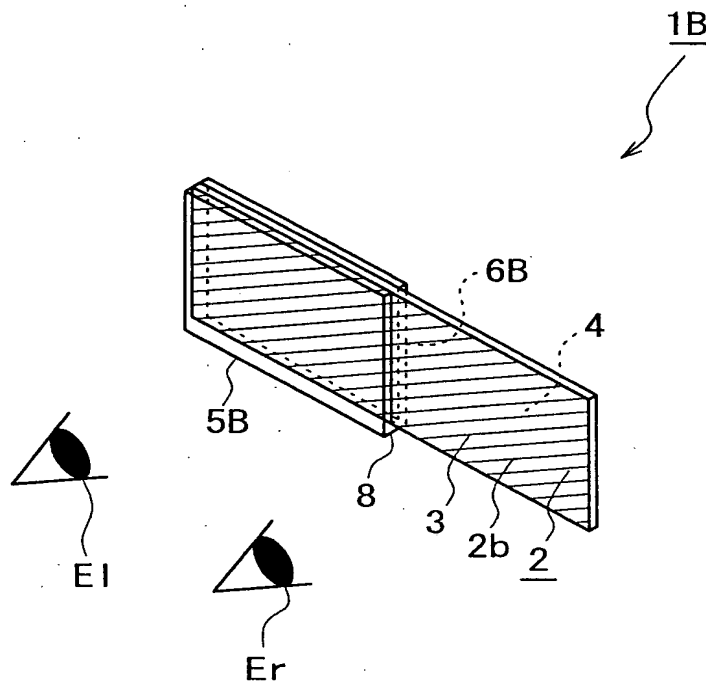


24 / 32

FIG. 24

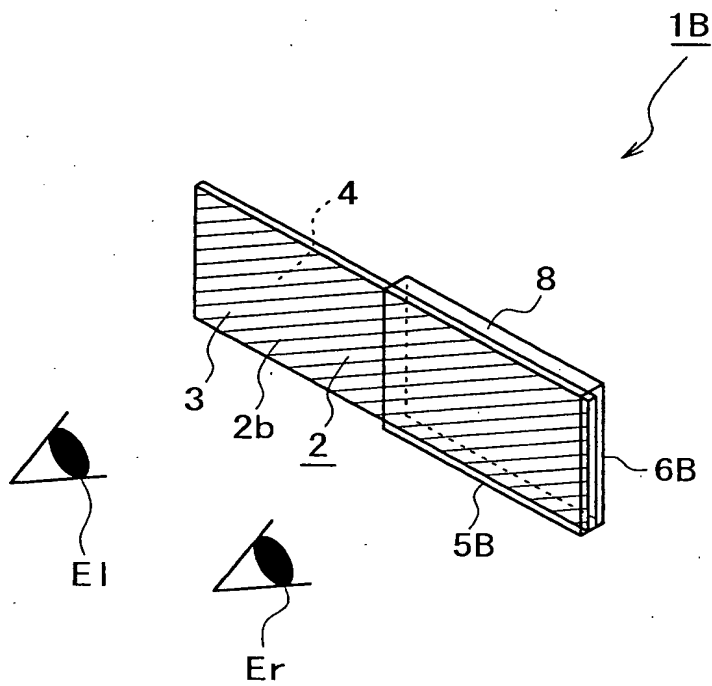

25/32

FIG. 25

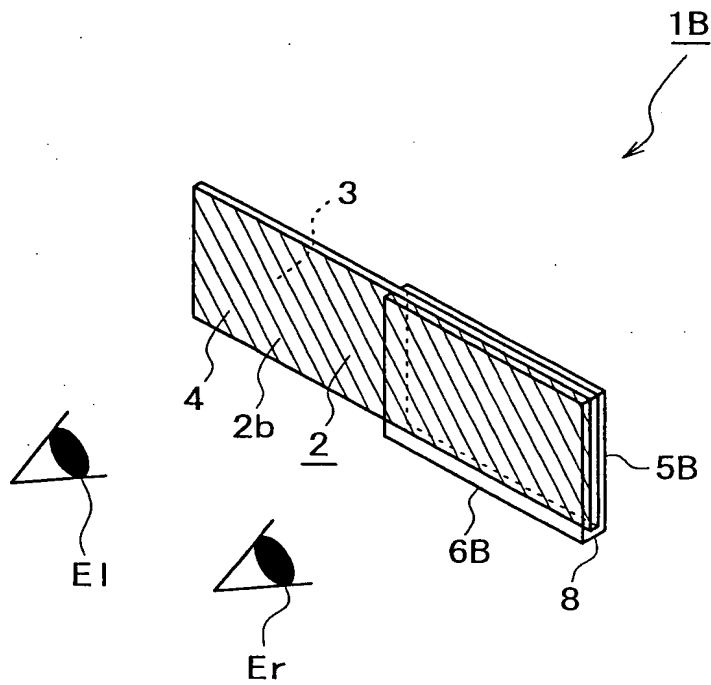

7254

IG. 27

		STEREOSCOPIC IMAGE DISPLAY APPARATUS			
		TYPE I	TYPE II	TYPE III	TYPE IV
POLARIZING EYEGLASS DEVICE	SERVICE CONDITION E				
	SERVICE CONDITION F				
	SERVICE CONDITION G				
	SERVICE CONDITION H				

28 / 32

FIG. 28



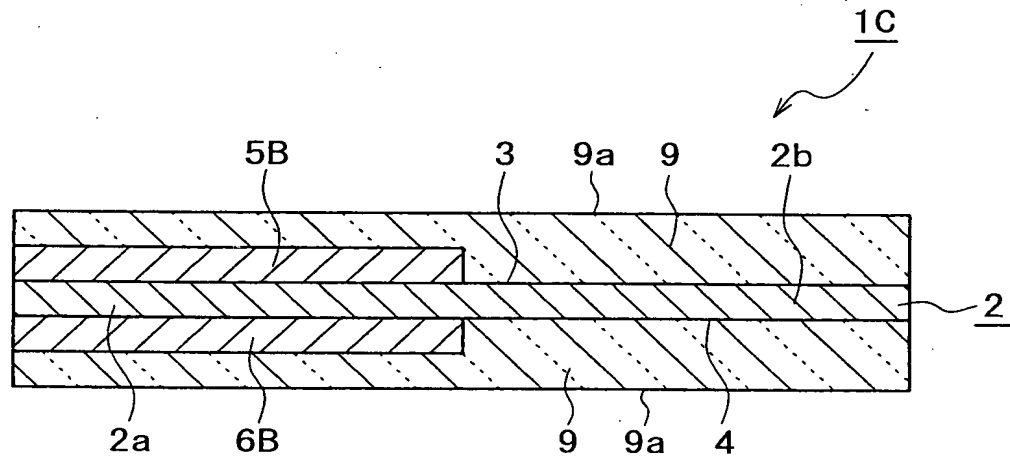


FIG. 29

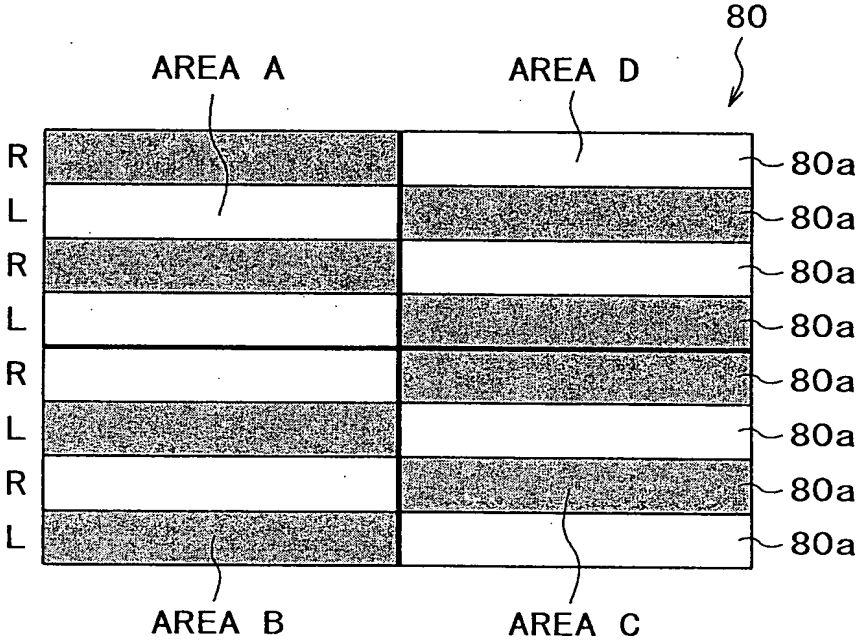


30 / 32

F I G. 3 0

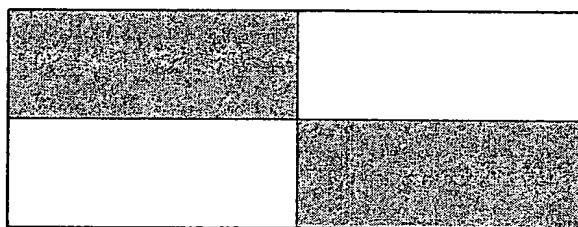


F I G. 3 1

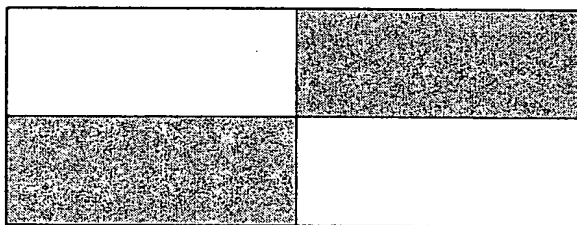

31/32

FIG. 32

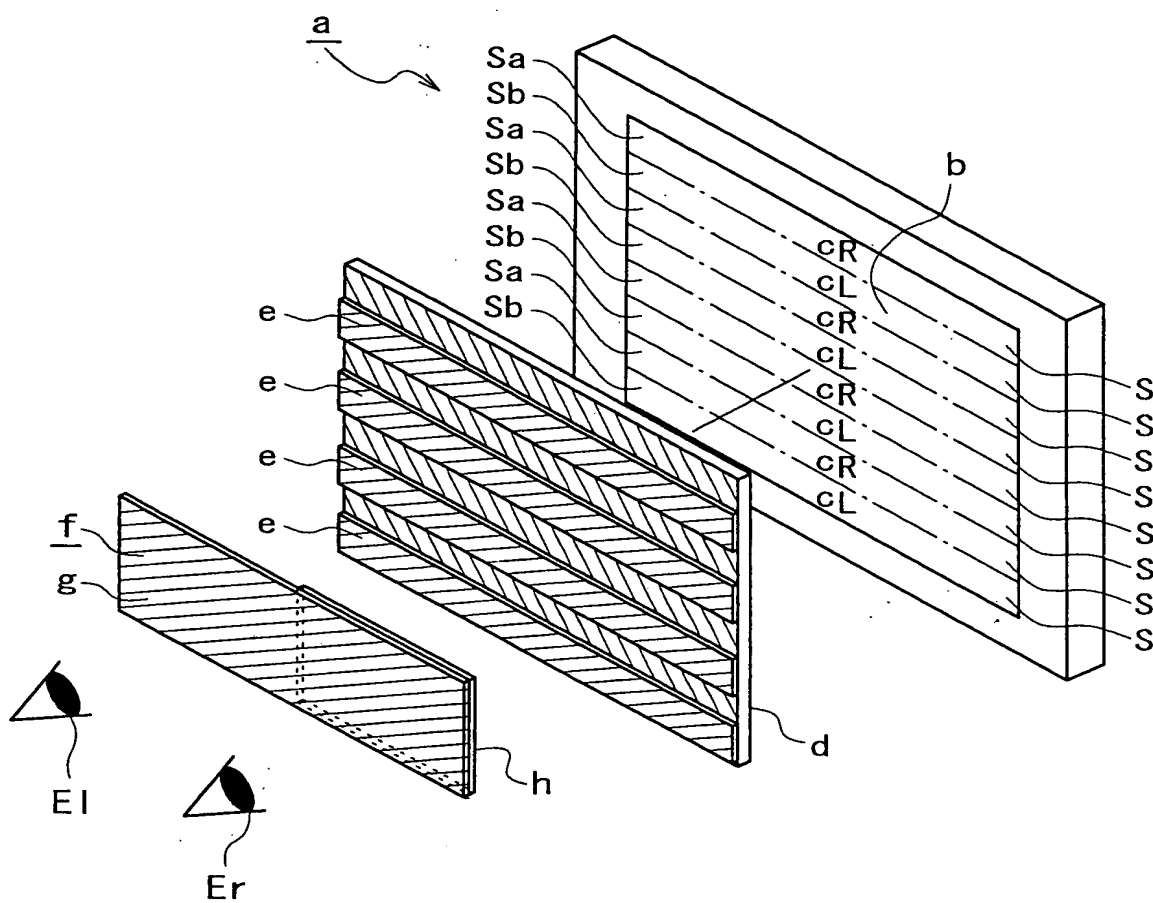

32 / 32

FIG. 33

